INSTALLATION REPORT

DataMaster DMT: 102606
Location: VPA
Calibration Date: 07/02/2012
Certification Date: 09/19/2012
Installation Date: 09/24/2012
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube    = 46.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.78 V
Cooler Voltage = 1.80 V
Bias Voltage   = 80 V
Chopper Freq   = 548 Hz

PUMP INFO
Flow Rate = 4.243 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0740   -0.0691
MIN(V)   -0.0756   -0.0711

FILTER INFO
Filter 1  -0.071  Zero = true
Filter 2   0.354  Zero = true
Filter 3   1.276  Zero = true

CALIBRATION CHECK
Xq  = 0.082  0.11%
```

INSTALLATION PASSED

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-58-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

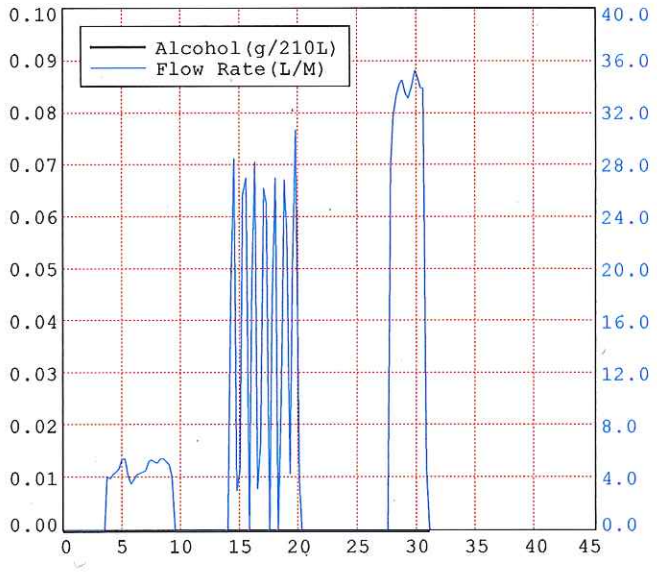

Performed by _____ **Date** 09/24/2012

Reviewed by _____ **Date** 10/1/2012