INSTALLATION REPORT

DataMaster DMT: 102706
Location: Stowe PD
Calibration Date: 03/18/2014
Certification Date: 03/18/2014
Installation Date: 03/18/2014
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.72 V
Cooler Voltage = 1.72 V
Bias Voltage   = 80 V
Chopper Freq   = 539 Hz

PUMP INFO
Flow Rate = 4.492 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1441    0.1478
MIN(V)   0.1427    0.1465

FILTER INFO
Filter 1   0.147  Zero = true
Filter 2   0.866  Zero = true
Filter 3   0.830  Zero = true

CALIBRATION CHECK
Xq  = 0.095  0.28%
```

Accuracy and Precision Check

Concentration = 0.099 g/210L
Lot # = 14-01-100
Range = 0.094 - 0.104
Average = 0.096 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

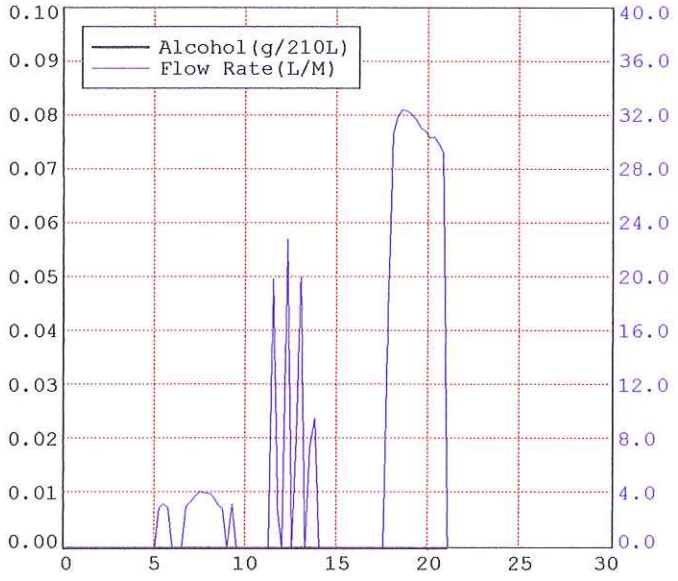

INSTALLATION PASSED

NIST Thermometer S/N 111814517 34.0°C RCD 3/18/14

Performed by RCD Date 03/18/2014

Reviewed by Date 3/19/2014