INSTALLATION REPORT

DataMaster DMT: 102906
Location: Orange SO
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 02/20/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 47.6°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.63 V
Cooler Voltage = 1.97 V
Bias Voltage   = 120 V
Chopper Freq   = 539 Hz

PUMP INFO
Flow Rate = 4.738 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0248    0.0274
MIN(V)   0.0234    0.0258

FILTER INFO
Filter 1   0.027  Zero = true
Filter 2   0.374  Zero = true
Filter 3   1.503  Zero = true

CALIBRATION CHECK
Xq  = 0.135  2.78%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-72-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

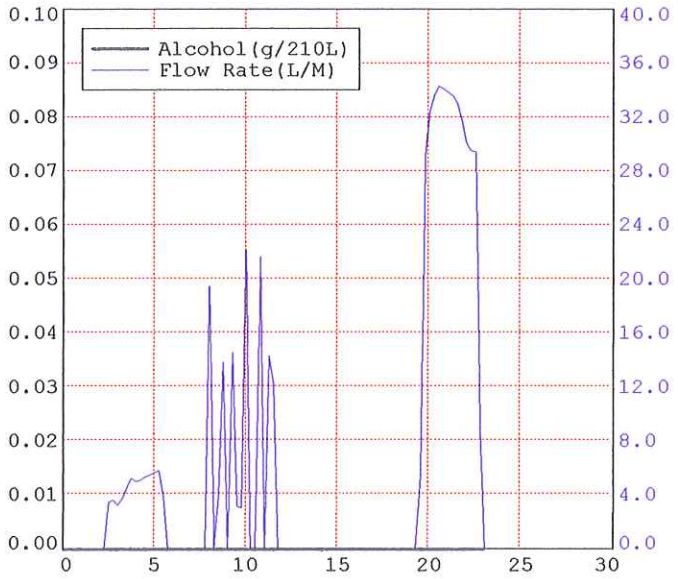

INSTALLATION PASSED

Performed by RCD 2/20/13 **Date** 02/20/2013

Reviewed by **Date** 2/20/2013

INSTALLATION REPORT

wrong agency entered during install
RCD 2/19/13

DataMaster DMT: 102906
Location: Orleans County SO
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 02/12/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 47.5°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.63 V
Cooler Voltage = 1.97 V
Bias Voltage   = 120 V
Chopper Freq   = 536 Hz

PUMP INFO
Flow Rate = 4.494 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0508    0.0537
MIN(V)   0.0492    0.0520

FILTER INFO
Filter 1   0.053  Zero = true
Filter 2   0.396  Zero = true
Filter 3   1.508  Zero = true

CALIBRATION CHECK
Xq  = 0.134  2.17%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-72-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

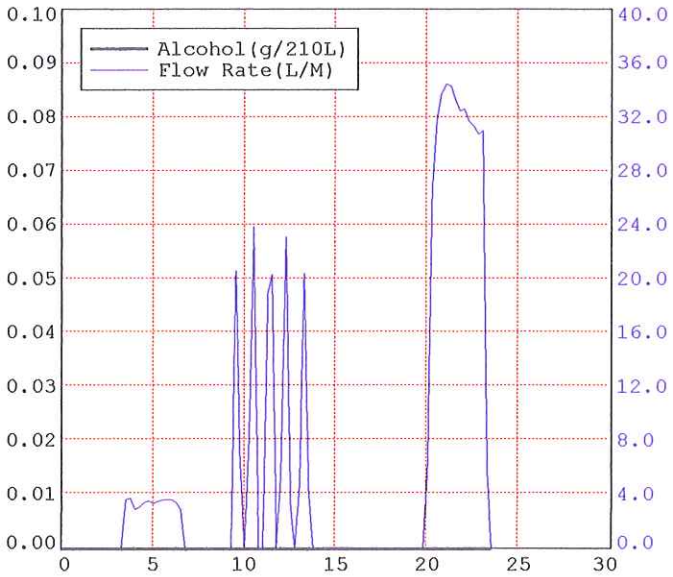

INSTALLATION PASSED

Performed by RCD 2/12/13 **Date** 02/12/2013

Reviewed by _____ **Date** _____

DIAGNOSTIC RESULT

DataMaster DMT: 102906
Location: Orange SO
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 10/27/2011
Test Date: 02/12/2013
Test Time: 10:35:34

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 46.9°C
Digital Sim = 34.1°C

SETTINGS
Lamp Voltage = 1.63 V
Cooler Voltage = 1.97 V
Bias Voltage = 120 V
Chopper Freq = 537 Hz

PUMP INFO
Flow Rate = 4.443 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	-0.0045	-0.0018
MIN(V)	-0.0061	-0.0037

FILTER INFO

Filter 1	-0.003	Zero = true
Filter 2	0.345	Zero = true
Filter 3	1.471	Zero = true

CALIBRATION CHECK
Xq = 0.134 2.17%

3 of 6 RCD

Status Record History

Status Date	Status Time	Test Type	Status Message
			4 of 6 RCD

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
12/29/2012	03:07:25	orange county sheriff dept	DAVID S EGGUM	0.131		0.096		

5 of 6 RD

INSTALLATION REPORT

DataMaster DMT: 102906
Location: Orange SO
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 02/20/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 33.9°C

SETTINGS
Lamp Voltage = 1.63 V
Cooler Voltage = 1.97 V
Bias Voltage = 120 V
Chopper Freq = 540 Hz

PUMP INFO
Flow Rate = 4.709 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0260	0.0276
MIN(V)	0.0234	0.0256

FILTER INFO
Filter 1 0.025 Zero = true
Filter 2 0.373 Zero = true
Filter 3 1.503 Zero = true

CALIBRATION CHECK
Xq = 0.135 2.78%

Accuracy and Precision Check

Concentration =
Lot # =
Range =
Average =
Std Dev =

INSTALLATION FAILED

Aborted by operator as I was not sure the correct agency was entered.
RCD
2/20/13

Performed by RCD **Date** 02/20/2013

Reviewed by _____ **Date** _____