ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 103206
Location: VFL
Calibration Date: 07/27/2012
Certification Date: 07/27/2012
Installation Date: 07/27/2012
RPC Date: 11/17/2014
Supervisor Name: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 43.9°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.90 V
Cooler Voltage = 1.93 V
Bias Voltage   = 120 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 4.085 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.5449    0.5468
MIN(V)   0.5423    0.5435

FILTER INFO
Filter 1   0.544  Zero = true
Filter 2   0.865  Zero = true
Filter 3   1.615  Zero = true

CALIBRATION CHECK
Xq  = 0.132  0.67%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 14-14-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

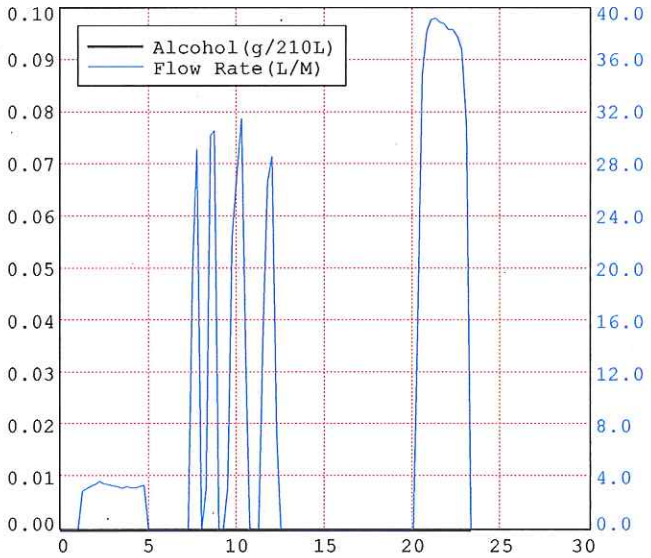

Performed by RCD Date 11/17/2014

Reviewed by Date 11/17/2014