ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT:	103509
Location:	Hardwick-Greensboro PD
Calibration Date:	07/29/2013
Certification Date:	07/29/2013
Installation Date:	07/30/2013
RPC Date:	06/21/2016
Supervisor Name:	STEVEN A MITCHELL

Diagnostic Results

```
VERSIONS
DMT: 2.00
PIC: 2.06
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 46.1°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.61 V
Cooler Voltage = 1.59 V
Bias Voltage   = 81 V
Chopper Freq   = 541 Hz

PUMP INFO
Flow Rate = 5.036 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2998    0.3008
MIN(V)   0.2978    0.2988

FILTER INFO
Filter 1   0.300  Zero = true
Filter 2   0.599  Zero = true
Filter 3   0.258  Zero = true

CALIBRATION CHECK
Xq  = 0.089  0.69%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 15-24-100
Range	= 0.094 - 0.104
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

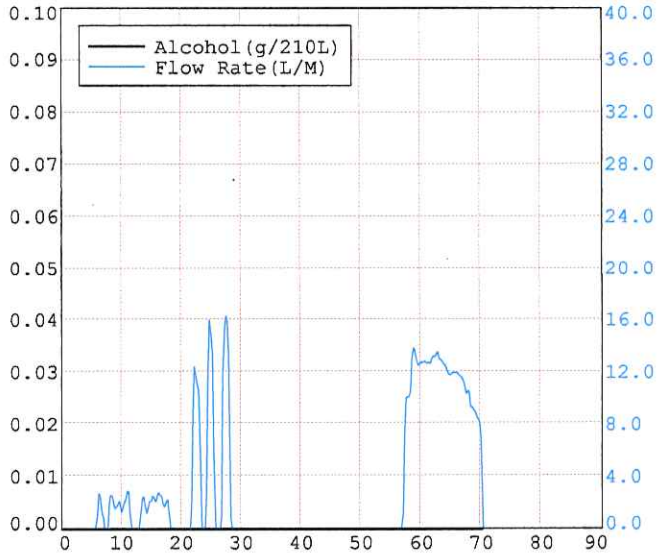

Performed by Steven Mitchell Date 06/21/2016 6/30/16

Reviewed by Date 6/22/16