INSTALLATION REPORT

DataMaster DMT: 103609
Location: St. Johnsbury PD
Calibration Date: 09/21/2011
Certification Date: 09/21/2011
Installation Date: 01/09/2013
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube    = 45.3°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.67 V
Cooler Voltage = 1.67 V
Bias Voltage   = 80 V
Chopper Freq   = 536 Hz

PUMP INFO
Flow Rate = 5.672 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.2423    0.2470
MIN(V)   0.2411    0.2457

FILTER INFO
Filter 1   0.246   Zero = true
Filter 2   0.466   Zero = true
Filter 3   0.125   Zero = true

CALIBRATION CHECK
Xq  = 0.081  0.74%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 12-90-100
Range	= 0.094 - 0.104
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

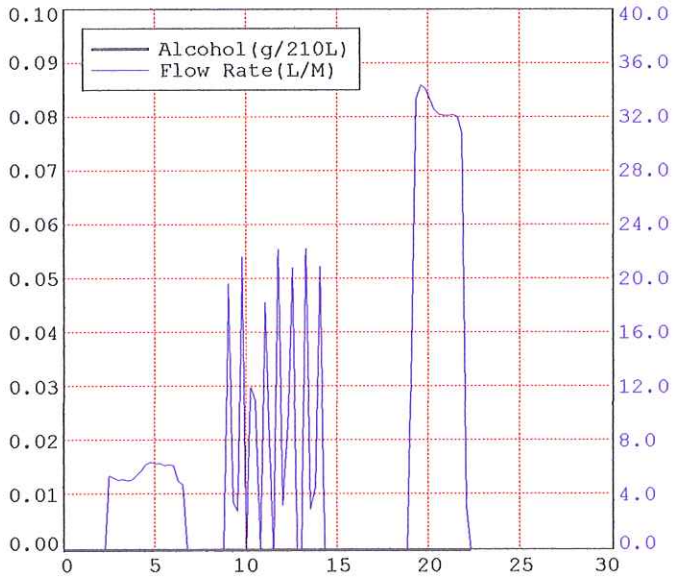

INSTALLATION PASSED

Performed by _____ **Date** 01/09/2013

Reviewed by _____ **Date** 1/9/2013