DataMaster Monthly Update Check-list

Department/Agency: **Winooski Police** _____DM serial #:104409

Date: **06/26/2012**

	Provided	None this month
Operators Logbook	X☐	☐
Maintenance Logbook	X☐	☐
Breath Summary Report	X☐	☐
Status Summary Report	X☐	☐
Calibration	☐	☐
Certification	☐	☐
Installation	☐	☐
Annual Preventative Maintenance	☐	☐
Routine Performance Check	X☐	☐
Simulator Solution Change	☐	☐
Other Reports	☐	☐

List other report type and date:

_____

_____

_____

Status Record History

Status Date	Status Time	Test Type	Status Message
05/09/2012	08:37:48	Check-In Confirmation Record	Simulator Out of Range
05/07/2012	16:43:45	DUI Subject Record	Simulator Out of Range
05/03/2012	21:14:09	Check-In Confirmation Record	Simulator Out of Range

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
06/21/2012	20:45:06	winooski police dept	RAINER J SHEEHAN	0.152		0.097		
06/16/2012	01:24:25	WINOOSKI PD	DEAN F FULLERTON	0.114		0.098		
06/08/2012	01:04:55	WINOOSKI PD	DEAN F FULLERON	REFUSED		0.098		
06/02/2012	23:52:37	WINOOSKI PD	RICHARD M HEBERT	0.149		0.099		
06/01/2012	03:17:07	WINOOSKI PD	MICHAEL E CRAM	0.100		0.100		
05/29/2012	21:20:09	COLCHESTER PD	JEREMY A WYSKIEL	0.119		0.099		
05/09/2012	08:36:13	WINOOSKI PD	KIMBERLY N BURBO			0.092		Simulator Out of Range
05/07/2012	16:42:09	WINOOSKI PD	JAMES P LEARNED			0.092		Simulator Out of Range
05/03/2012	21:12:37	WINOOSKI PD	JAMES V CHARKALIS			0.092		Simulator Out of Range

DATAMASTER DMT OPERATOR USE LOG

Winnsboro PD
Department/Agency

104409
DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
3-27-12	Hebert	Douglas Cadieux	.096	.095
3/28/12	Davis	Anthony Harvey	.096	.096
4-3-12	Dewey	James Hance	.095	—
4-14-12	Adams	Tyler Meigs	.094	
	Out of Range			
4-15-12	Learned	Julie DeSaulels	.100	
4-18-12	Adams	Lucy Freeman	.094	
	Out of Range			
4-20-12	CRAM	Jordan Pautik	.100	
4-28-12	Adams	Corran Soy	.093	.093
5-7-12	Learned	Dale Ryan	.100	
5-6-12	Burbo	Dale Ryan	.092	Out of Range
5/18/12	SOLUTION CHANGE NOTES		.102	
5/29/12	Wyskiel, Jeremy	Williams, Edward	.099	
6-1-12	CRAM	Prior, Kristina	.100	
6-3-12	Hebert	Eric Martin	.101	
6-8-12	Fullerton	Thomas Finnegan	.098	
6-16-12	Fullerton	Zach Allen	.098	
6/21/12	SHEEHAN	Ty J. Codd	.098	

ALC 603 Rev 3 08/11

DATAMASTER DMT OPERATOR USE LOG

WEINDSKE PD
Department/Agency

1.04409
DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
6/25	NOKES · 914	RPC	.100	

DATAMASTER DMT MAINTENANCE LOG

Winooski PD
Department/Agency

104409
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
12/23/11	**DataMaster Simulator Solution** Lot # 12-38-100 $EtOH_{aq}$ Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 11/17/2011 Expires: 11/17/2012 OPENED: 12/23/11 [For RP ... ce Label Here] Installed	A. B[illegible]
1/13/12	**DataMaster Simulator Solution** Lot # 12-38-100 $EtOH_{aq}$ Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 11/17/2011 Expires: 11/17/2012 OPENED: 1/13/12 [For RP ... ce Label Here] CHANGE	NOKES 914
1/16/12	Finished solution change started by J. Nokes	Hebert 904
2/26/12	**DataMaster Simulator Solution** Lot # 12-45-100 $EtOH_{aq}$ Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 12/12/2011 Expires: 12/12/2012 OPENED: 2/26/12 [For RPC ... e Label Here]	NOKES 914
2/26/12	RPC	NOKES 914
5/18/12	**DataMaster Simulator Solution** Lot # 12-64-100 $EtOH_{aq}$ Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/17/2012 Expires: 02/17/2013 OPENED: 5/18/12 [For RP ... ace Label Here]	NOKES 914
6/7/12	Software Update & lock change	[illegible]

ALC 803 REV 03 08/2011

DATAMASTER DMT MAINTENANCE LOG

Wisinski PD
Department/Agency

104409
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/25/12	[For RPC or **DataMaster Simulator Solution** Lot # 12-72-100 EtOHaq Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 04/24/2012 Expires: 04/24/2013 OPENED: 6/25/12 ...abel Here]	NOKES 914
6/25/12	RPC	NOKES 914
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 104409
Location: Winooski PD
Calibration Date: 12/19/2011
Certification Date: 12/20/2011
Installation Date: 12/23/2011
RPC Date: 06/26/2012
Supervisor Name: JASON R NOKES

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.72 V
Cooler Voltage = 1.72 V
Bias Voltage = 80 V
Chopper Freq = 536 Hz

PUMP INFO
Flow Rate = 6.173 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.1841	0.1868
MIN(V)	0.1823	0.1854

FILTER INFO
Filter 1 0.185 Zero = true
Filter 2 0.423 Zero = true
Filter 3 0.576 Zero = true

CALIBRATION CHECK
Xq = 0.081 1.75%

Accuracy and Precision Check

Concentration = 0.100 g/210L
Lot # = 12-72-100
Range = 0.095 - 0.105
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

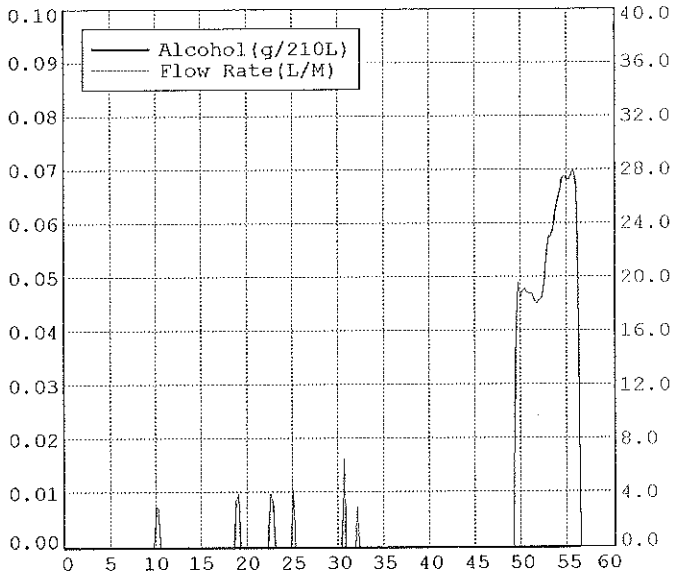

Routine Performance Check Passed

Performed by Jason R Nokes 914 Date 06/26/2012

Reviewed by Date 6/28/12

6/28/2012