

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 104409
Location: Winooski PD
Calibration Date: 12/19/2011
Certification Date: 12/20/2011
Installation Date: 12/23/2011
RPC Date: 07/01/2014
Supervisor Name: RICHARD M HEBERT

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.72 V
Cooler Voltage = 1.72 V
Bias Voltage = 80 V
Chopper Freq = 539 Hz

PUMP INFO

Flow Rate = 6.152 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.3187	0.3209
MIN (V)	0.3173	0.3195

FILTER INFO

Filter	Value	Zero
Filter 1	0.320	Zero = true
Filter 2	0.561	Zero = true
Filter 3	0.713	Zero = true

CALIBRATION CHECK

Xq = 0.081 1.645

Routine Performance Check Passed

Accuracy and Precision Check


Concentration	0.099 g/210L
Lot #	13-16-100
Range	0.094 - 0.104
Average	0.098 g/210L
Std Dev	0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

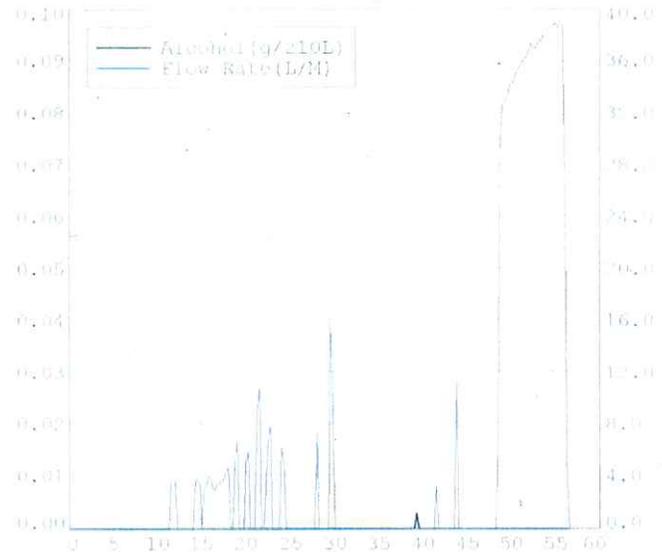

See attached passing sample acceptance. REC 8/13/14

Performed by

R.M. Hebert

Date

07/01/2014

Reviewed by

JH

Date

8/13/14

TEGA
8/13/2014

DMT Serial Number #104409

Page 1 of 1

07/01/2014 3:51 PM

Page 1 of 6 REC

Driscoll, Rob

From: Rick Hebert <rhebert@winooskipolice.com>
Sent: Monday, August 11, 2014 1:49 PM
To: Driscoll, Rob
Subject: Re: FW: Winooski June RPC
Attachments: CheckIntest.pdf

Hi Rob,

Sorry for the delay I was away at training. I just did a check in test. I hope this is what you need.

Rick

Acting Deputy Chief Rick Hebert
Winooski Police Department
27 West Allen Street
Winooski, VT 05404
(Tel) - 802-655-0221 x29
(Fax)- 802-655-6427

On Wed, Aug 6, 2014 at 7:05 AM, Driscoll, Rob <Rob.Driscoll@state.vt.us> wrote:

Did you have a chance to complete the "check in" yet?

Thanks,

Rob

From: Driscoll, Rob
Sent: Friday, July 11, 2014 8:31 AM
To: DPS - Rhebert-ForwardAddress
Subject: RE: Winooski June RPC

Rick,

In looking at the June RPC I noticed a small "blip" in the alcohol line during the "suck-back test". Can you please perform a "Check-In" including all 4 breath samples (shallow, intermittent, suck back, and 1.5 liter alcohol free sample). Remember when performing the "suck-back test" that you are only sucking VERY gently to check the one way valve in

the breath tube. This valve is a small rubber flap that closes when air is "sucked back" and requires minimal backwards air pressure to check. If you have any questions please feel free to contact me.

Regards,

Rob

Robert Driscoll

Vermont Forensics Laboratory

103 South Main Street

Waterbury, VT 05671

Electronics Technician

Rob.Driscoll@state.vt.us

Desk: [\(802\) 241-5817](tel:(802)241-5817)

Cell: [\(802\) 585-0123](tel:(802)585-0123)

From: Rick Hebert [<mailto:rhebert@winooskipolice.com>]

Sent: Friday, July 11, 2014 8:26 AM

To: Driscoll, Rob

Subject: Winooski June RPC

Acting Deputy Chief Rick Hebert

Winooski Police Department

27 West Allen Street

From: Rick Hebert

Sent: Friday, July 11, 2014 8:26 AM

To: Driscoll, Rob

Subject: Winooski June RPC

Winooski, VT 05404

(Tel) - 802-655-0221 x29

(Fax)- 802-655-6427

27 00

27 00

Winooski

(Tel) - 802-655-0221

(Fax) - 802-655-6427

27 00

27 00

Winooski

(Tel) - 802-655-0221

(Fax) - 802-655-6427

27 00

27 00

Winooski

(Tel) - 802-655-0221

(Fax) - 802-655-6427



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 104409
Location: Winooski PD
Certification Date: 12/20/2011
Installation Date: 12/23/2011


Date: 08/11/2014
Time: 13:31:18

SUBJECT NAME:
TEST T TEST
DOB: 01/01/1970 AGE: 44
GENDER: M
LICENSE #: 81637938 VT

TEST OPERATOR NAME:
RICHARD M HEBERT
AGENCY: WINOOSKI PD

BLANK TEST	0.000	13:32
CALIBRATION CHECK	PASSED	13:32
SIMULATOR VAPOR 34.1°C	0.096	13:32
SUBJECT SAMPLE (Vol=3.1L)	0.000	13:34
BLANK TEST	0.000	13:35

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.099
Sim. Vapor Range 0.094 - 0.104
Lot #: 13-16-100

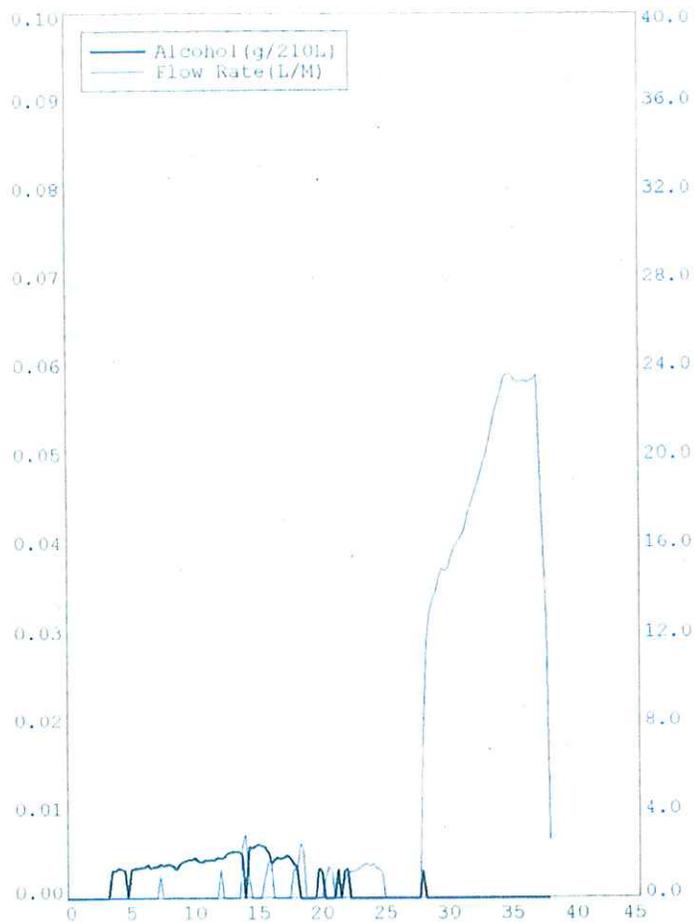



CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 104409
Location: Winooski PD
Certification Date: 12/20/2011
Installation Date: 12/23/2011

Date: 08/12/2014
Time: 06:45:09

SUBJECT NAME:
TEST TEST
DOB: 06/05/1979 AGE: 35
GENDER: M
LICENSE #: 000000 VT

TEST OPERATOR NAME:
ROBERT DRISCOLL
AGENCY: VFL

BLANK TEST	0.000	06:46
CALIBRATION CHECK	PASSED	06:46
SIMULATOR VAPOR 34.0°C	0.096	06:46
SUBJECT SAMPLE (Vol=1.7L)	0.000	06:47
BLANK TEST	0.000	06:48

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.099
Sim. Vapor Range 0.094 - 0.104
Lot #: 13-16-100

