INSTALLATION REPORT

DataMaster DMT: 104709
Location: VPA
Calibration Date: 04/01/2013
Certification Date: 04/02/2013
Installation Date: 04/16/2014
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.5
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube    = 48.1°C
Digital Sim    = 33.8°C

SETTINGS
Lamp Voltage   = 1.70 V
Cooler Voltage = 1.67 V
Bias Voltage   = 80 V
Chopper Freq   = 532 Hz

PUMP INFO
Flow Rate = 5.694 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0134   -0.0102
MIN(V)   -0.0154   -0.0116

FILTER INFO
Filter 1  -0.010  Zero = true
Filter 2   0.791  Zero = true
Filter 3   0.802  Zero = true

CALIBRATION CHECK
Xq  = 0.082  0.53%
```

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-19-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0004

RF Detection Test

Passed

Sample Acceptance Test

Passed

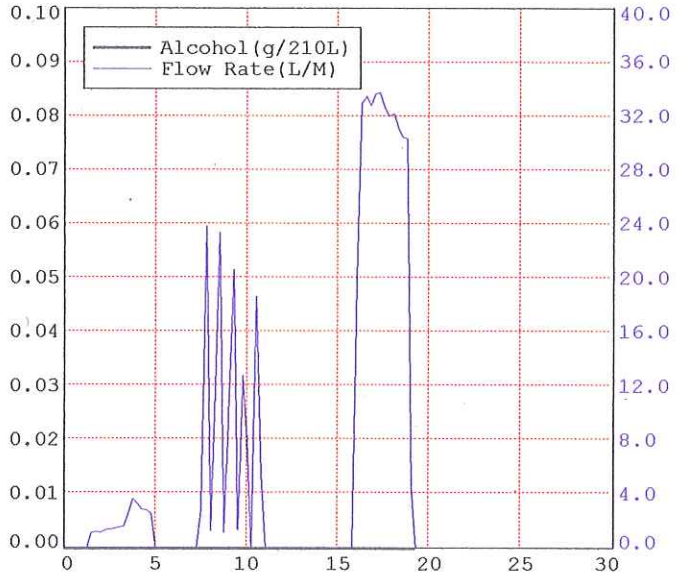

INSTALLATION PASSED

Performed by RCD Date 04/16/2014

Reviewed by Date 4/21/2014