

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 104909
 Location: Williston PD
 Calibration Date: 12/07/2011
 Certification Date: 12/08/2011
 Installation Date: 12/21/2011
 RPC Date: 10/20/2013
 Supervisor Name: BRIAN J CLAFFY

Diagnostic Results

VERSIONS

DMT: 1.01
 PIC: 2.05
 Modem: 2.4
 Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
 Breath Tube = 48.1°C
 Digital Sim = 33.9°C

SETTINGS

Lamp Voltage = 1.78 V
 Cooler Voltage = 1.72 V
 Bias Voltage = 81 V
 Chopper Freq = 542 Hz

PUMP INFO

Flow Rate = 5.661 L/M

DETECTOR INFO

PUMP ON OFF
 MAX(V) 0.0266 0.0283
 MIN(V) 0.0242 0.0268

FILTER INFO

Filter 1 0.026 Zero = true
 Filter 2 0.723 Zero = true
 Filter 3 0.364 Zero = true

CALIBRATION CHECK

Xq = 0.083 1.37%

Accuracy and Precision Check


Concentration = 0.099 g/210L
 Lot # = 13-04-100
 Range = 0.094 - 0.104
 Average = 0.099 g/210L
 Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

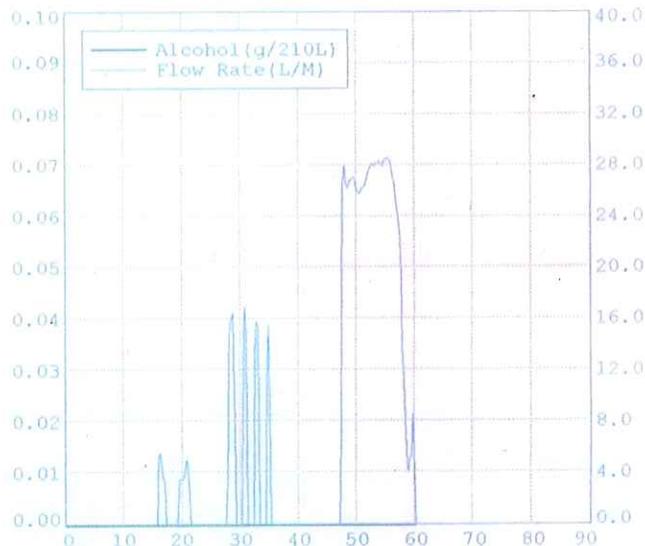

Routine Performance Check Passed

Performed by [Signature]

Date 10/20/2013

Reviewed by [Signature]

Date 10/28/13

DMT Serial Number #104909

Page 1 of 1

10/20/2013 7:26 AM

page 1 of 4 ROD

SOLUTION CHANGE

DataMaster DMT: 104909
Location: Williston PD
Date: 10/20/2013
Performed by: BRIAN J CLAFFY



Accuracy and Precision Check

Concentration = 0.099 g/210L
Lot # = 13-04-100
Range = 0.094 - 0.104
Average = 0.098 g/210L
Std Dev = 0.0000

Simulator Temperature: 33.9°C

Performed by

A handwritten signature in blue ink, appearing to read "B. Claffy", written over a horizontal line.

Date

10/20/2013

Driscoll, Rob

From: Lavoie, Michael
Sent: Monday, October 28, 2013 9:52 AM
To: Driscoll, Rob
Subject: RE: DataMaster DMT October RPC Due
Attachments: OCT RPC.jpg

Yes it was done Brian Claffy did it.

Michael Lavoie
Detective
Williston Police
7928 Williston Road
Williston, Vermont 05495

802 878 6611
802 373 9003 C
802 872 1124 fax

From: Driscoll, Rob
Sent: Monday, October 28, 2013 8:34 AM
To: Lavoie, Michael
Subject: RE: DataMaster DMT October RPC Due

Michael,

You sent me a "Solution Change" printout and not a "Routine Performance Check"? Have you completed the RPC? The solution change is the first step in completing an RPC, but you do not need to perform a solution change protocol (just the RPC protocol). IF you have any questions please refer to your DMT supervisor manual or contact me.

Regards,
Rob

From: Lavoie, Michael
Sent: Monday, October 28, 2013 8:24 AM
To: Driscoll, Rob
Subject: RE: DataMaster DMT October RPC Due

Michael Lavoie
Detective
Williston Police
7928 Williston Road
Williston, Vermont 05495

802 878 6611
802 373 9003 C
802 872 1124 fax

From: Driscoll, Rob

Sent: Monday, October 28, 2013 8:16 AM

To: Deslauriers, Katherine; Steeves, Matthew; Harvey, Allison; Taylor, Stephanie; Ambroz, Todd; Ravelin, Paul; Campbell, Greg; Reeve, Michael; Allen, Blake; Abell, Dustin; Gauld, Bruce; Hebert, MaryBeth; Simpson, Tom; Leonard, Anthony; Norton, Christopher; Noyes, Jeffrey; Marceau, Andrew; Kirkpatrick, Troy; Moulton, Charles; Cushing, Blake; Quesnel, Christopher; Bennett, Daniel F; Kinney, Tyson; Howard, Joel; Noblet, Jason; Sly, John; MacFarlane, Jonathan; Brooks, Philip; Gero, Michael; Cochran, Aaron; Herbes, Cassandra; Winn, Charles; Greenough, Richard; Adams, Jonathan; Benoit, Richard; Nokes, Jason; King, Richard; Lavoie, Michael; Claffy, Brian; Gilbert, Donald; Ellis, Holly; LaFlam, Jody; Rainault, Gil; Kevin Emilio; Christopher Mason; Jason Covey; Reeve, Michael; Dominic Brodeur; Dwayne Mellis; Paul Fabiani

Cc: Conti, Trisha

Subject: DataMaster DMT October RPC Due

Our records indicate that you have not yet performed the October RPC for your DataMaster DMT. If this is not completed before the end of October, the instrument will automatically be removed from service until such time as a passing RPC is completed. The instrument will display "*Routine Performance Check Required*". Please submit a color copy of your results to us via e-mail or mail at your earliest convenience.

If you have any questions, please contact me.

Regards,

Rob

Robert Driscoll
Vermont Forensics Laboratory
103 South Main Street
Waterbury, VT 05671
Electronics Technician
Rob.Driscoll@state.vt.us
Desk: (802) 241-5817
Cell: (802) 585-0123