ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 104909
Location: Williston PD
Calibration Date: 12/07/2011
Certification Date: 12/08/2011
Installation Date: 12/21/2011
APM Date: 11/19/2015
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.4°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.79 V
Cooler Voltage = 1.72 V
Bias Voltage   = 81 V
Chopper Freq   = 542 Hz

PUMP INFO
Flow Rate = 5.841 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1559    0.1573
MIN(V)   0.1541    0.1559

FILTER INFO
Filter 1   0.156  Zero = true
Filter 2   0.833  Zero = true
Filter 3   0.494  Zero = true

CALIBRATION CHECK
Xq  = 0.084  2.22%
```

APM PASSED

Simulator Vapor Test

Concentration = 0.100 g/210L
Lot # = 15-07-100
Range = 0.095 - 0.105
Simulator Vapor = 0.096 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

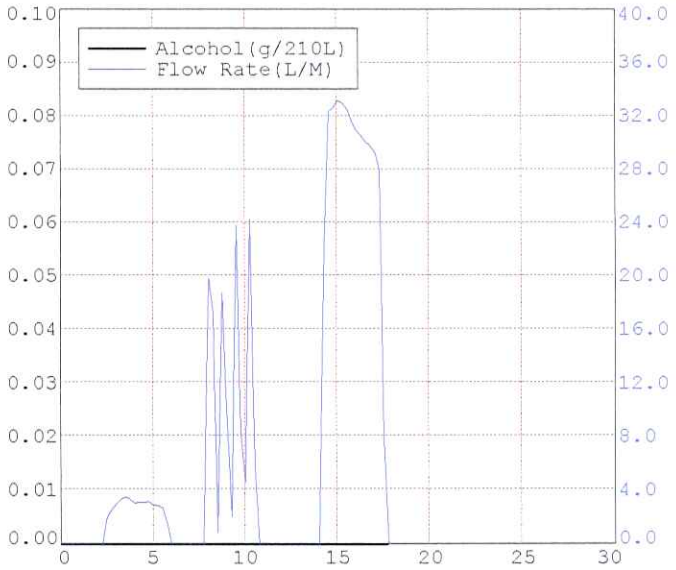

NIST Thermometer s/n 111814367 34.1°C RCD 11/19/15

Performed by RCD Date 11/19/2015

Reviewed by Date 11/24/15