ANNUAL PREVENTATIVE MAINTENANCE

DataMaster DMT: 122106
Location: Vergennes PD
Calibration Date: 01/03/2012
Certification Date: 01/04/2012
Installation Date: 01/12/2012
APM Date: 01/03/2013
Performed by: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube    = 45.6°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.72 V
Cooler Voltage = 1.79 V
Bias Voltage   = 80 V
Chopper Freq   = 529 Hz

PUMP INFO
Flow Rate = 5.150 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.1244    0.1291
MIN(V)   0.1226    0.1274

FILTER INFO
Filter 1   0.128  Zero = true
Filter 2   0.514  Zero = true
Filter 3   0.783  Zero = true

CALIBRATION CHECK
Xq  = 0.086  0.20%
```

APM PASSED

Simulator Vapor Test

Concentration	= 0.098 g/210L
Lot #	= 12-73-100
Range	= 0.093 - 0.103
Simulator Vapor	= 0.097 g/210L

RF Detection Test

Passed

Sample Acceptance Test

Passed

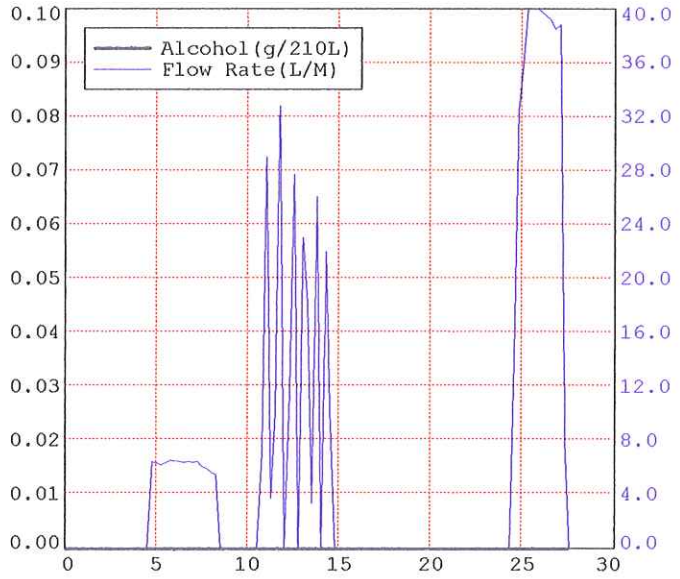

Performed by _____ Date 01/03/2013

Reviewed by _____ Date 1/7/2013