ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 123206
Location: Middlebury PD
Calibration Date: 01/03/2012
Certification Date: 01/04/2012
Installation Date: 01/12/2012
RPC Date: 02/11/2014
Supervisor Name: KEVIN A EMILIO

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 44.8°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.73 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 539 Hz

PUMP INFO
Flow Rate = 4.566 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3024    0.3073
MIN(V)   0.3002    0.3055

FILTER INFO
Filter 1   0.307  Zero = true
Filter 2   0.656  Zero = true
Filter 3   1.603  Zero = true

CALIBRATION CHECK
Xq  = 0.081  0.00%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 13-16-100
Range	= 0.094 - 0.104
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

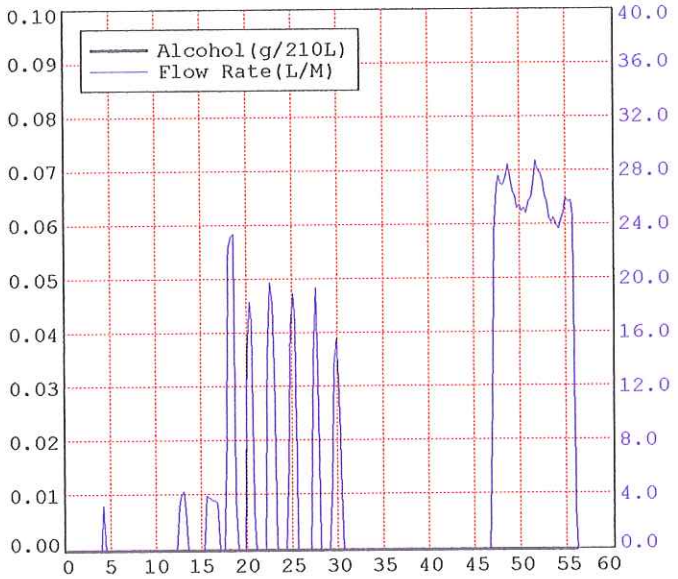

Performed by _____ Date 02/11/2014

Reviewed by _____ Date 2/19/14

2/19/2014

DMT Serial Number #123206

02/11/2014 7:04 PM