ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 123306
Location: New Haven VSP
Calibration Date: 12/23/2011
Certification Date: 12/23/2011
Installation Date: 01/03/2013
RPC Date: 01/26/2014
Supervisor Name: ALLISON M HARVEY

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.66 V
Cooler Voltage = 1.77 V
Bias Voltage = 80 V
Chopper Freq = 544 Hz

PUMP INFO
Flow Rate = 4.753 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.4681	0.4718
MIN (V)	0.4667	0.4699

FILTER INFO

Filter 1	0.471	Zero = true
Filter 2	0.917	Zero = true
Filter 3	1.493	Zero = true

CALIBRATION CHECK
Xq = 0.126 0.07%

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.098 g/210L
Lot #	= 13-03-100
Range	= 0.093 - 0.103
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

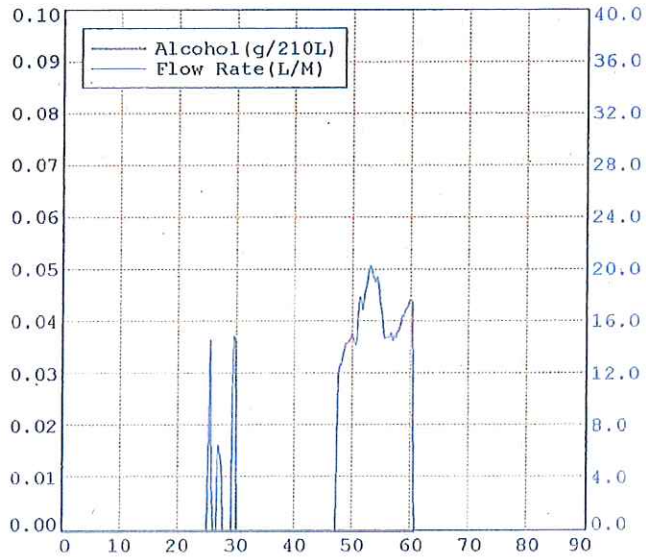

See check-in for passing sample acceptance. RCO 2/6/14

Performed by Allison M Harvey Date 01/26/2014

Reviewed by Date 2/6/14

2/12/2014

Page 1 of 2 RO

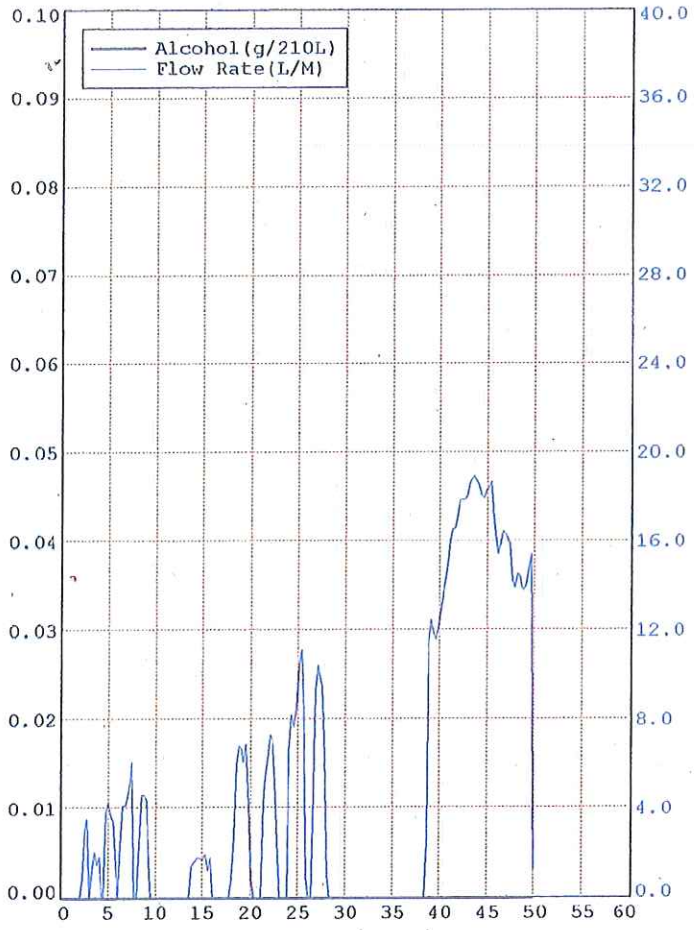

CHECK-IN CONFIRMATION TEST

STATE OF VERMONT

DataMater DMT: 123306
Location: New Haven VSP
Certification Date: 12/23/2011
Installation Date: 01/03/2013

Date: 02/02/2014
Time: 15:47:06

SUBJECT NAME:
TEST TEST
DOB: 01/01/2000 AGE: 14
GUARDIAN PRESENT: N
GENDER: F
LICENSE #: 12345678 VT

TEST OPERATOR NAME:
ALLISON M HARVEY
AGENCY: spc2

BLANK TEST	0.000	15:48
CALIBRATION CHECK	PASSED	15:48
SIMULATOR VAPOR 33.9°C	0.100	15:48
SUBJECT SAMPLE (Vol=2.9L)	0.000	15:49
BLANK TEST	0.000	15:50

All alcohol values reported in g/210L
Sim. Vapor Concentration 0.098
Sim. Vapor Range 0.093 - 0.103
Lot #: 13-03-100

Page 2 of 2 KCD