INSTALLATION REPORT

DataMaster DMT: 300151
Location: Wilmington PD
Calibration Date: 12/07/2011
Certification Date: 12/08/2011
Installation Date: 08/10/2012
Installed by: ROBERT DRISCOLL

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube    = 41.2°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.71 V
Cooler Voltage = 1.73 V
Bias Voltage   = 80 V
Chopper Freq   = 539 Hz

PUMP INFO
Flow Rate = 4.847 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.4636    0.4665
MIN(V)   0.4620    0.4646

FILTER INFO
Filter 1   0.466  Zero = true
Filter 2   1.176  Zero = true
Filter 3   0.734  Zero = true

CALIBRATION CHECK
Xq  = 0.087  2.36%
```

TLC

Accuracy and Precision Check

Concentration	= 0.098 g/210L
Lot #	= 12-73-100
Range	= 0.093 - 0.103
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

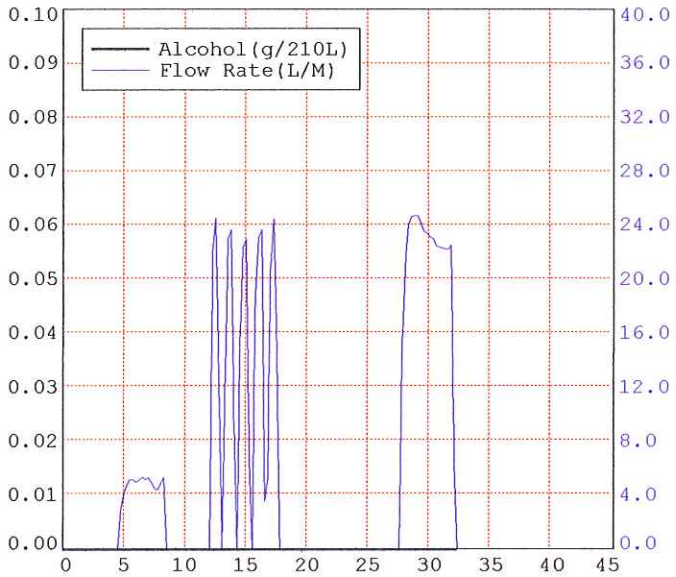

INSTALLATION PASSED

Performed by _____ Date 08/10/2012

Reviewed by _____ Date 8/13/2012