ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 300386
Location: Franklin County SO Richford
Calibration Date: 05/29/2013
Certification Date: 05/29/2013
Installation Date: 07/02/2013
RPC Date: 10/14/2015
Supervisor Name: ROBERT DRISCOLL

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 45.9°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.62 V
Cooler Voltage = 1.67 V
Bias Voltage   = 80 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 5.211 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0654    0.0685
MIN(V)   0.0630    0.0661

FILTER INFO
Filter 1   0.066  Zero = true
Filter 2   0.745  Zero = true
Filter 3   0.171  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.94%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.099 g/210L
Lot #	= 15-12-100
Range	= 0.094 - 0.104
Average	= 0.095 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

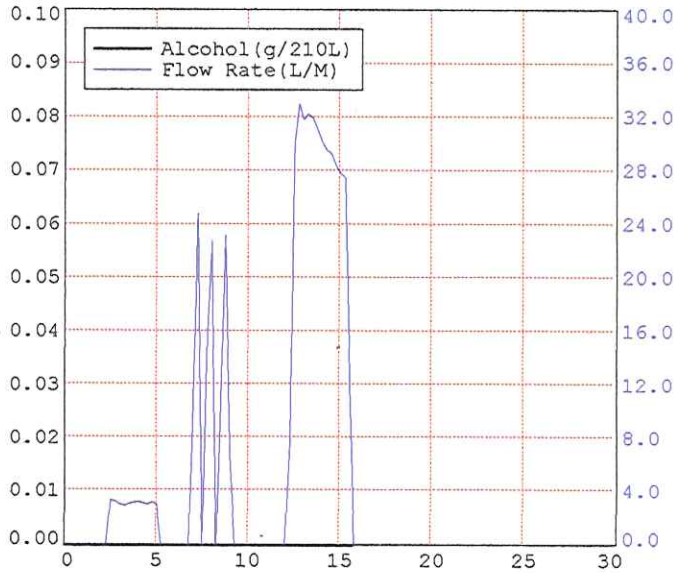

Performed by RCO Date 10/14/2015 10/27/15

Reviewed by AB Date 10/27/15

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 300386
Location: Franklin County SO Richford
Calibration Date: 05/29/2013
Certification Date: 05/29/2013
Installation Date: 07/02/2013
RPC Date: 10/08/2015
Supervisor Name: NATHAN J VAILLANCOURT

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 45.0°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.62 V
Cooler Voltage = 1.66 V
Bias Voltage   = 80 V
Chopper Freq   = 537 Hz

PUMP INFO
Flow Rate = 5.250 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)    0.0598    0.0626
MIN(V)    0.0579    0.0610

FILTER INFO
Filter 1   0.062  Zero = true
Filter 2   0.741  Zero = true
Filter 3   0.167  Zero = true

CALIBRATION CHECK
Xq  = 0.083  0.73%

Filter Wheel Error
```

Routine Performance Check Failed

Performed by Nathan Vaillancourt Date 10/08/2015

Reviewed by _____ Date _____

2 of 3 RO

Status Record History

Status Date	Status Time	Test Type	Status Message
01/24/2015	18:08:17	Check-In Confirmation Record	Simulator Out of Range
09/12/2015	02:26:39	DUI Subject Record	Simulator Out of Range
09/12/2015	02:29:39	DUI Subject Record	Simulator Out of Range
10/08/2015	23:21:20	RPC Record	Diagnostic Check Failed

3 of 3 ROS